



महाराष्ट्र शासन
शासकीय वैद्यकीय महाविद्यालय, धाराशिव
GOVERNMENT MEDICAL COLLEGE, DHARASHIV
कोविड-१९ इमारत, जिल्हा रुग्णालय आवार, धाराशिव. (महाराष्ट्र) 413 501
e-mail: deangmcosmanabad@gmail.com



जा.क्र./शावैमधा/भांडार/रा.यो./दरपत्रके/ 108 /२०२५

दिनांक: ०९/०९/२०२५

प्रति,

विषय :- सन २०२४-२५ या वित्तीय वर्षाकरिता राज्य योजना (स्टेट-प्लॅन) अंतर्गत प्रदान करण्यात आलेल्या प्रशासकीय मान्यते मधील यंत्रसामुग्री व साधनसामुग्री खरेदीकरिता दरपत्रके प्रसिध्द करणेबाबत.
संदर्भ :- दिनांक ०६/०९/२०२५ रोजीची मंजूर कार्यालयीन टिप्पणी.

उपरोक्त विषयास अनुसरुन कळविण्यात येते की नवनिर्मित शासकीय वैद्यकीय महाविद्यालय, धाराशिव या संस्थेतील औषधवैद्यकशास्त्र/ स्त्रीरोग व प्रसुतीशास्त्र/ कान-नाक-घसाशास्त्र विभागास वैद्यकीय अभ्यासक्रम व रुग्णसेवेकरिता विविध यंत्रसामुग्री व साधनसामुग्री खरेदी करण्याची संस्थेस आवश्यकता आहे.

तरी मागणीप्रमाणे उच्च दर्जाची यंत्रसामुग्री व साधनसामुग्री खरेदी करुन पुरवठा/प्रस्थापित करणेकामी पात्र निविदा धारकांकडुन विहित अटी व शर्तीना अनुसरुन दि. ०९/-०९-/२०२५ ते दि. १६/-०९-/२०२५ कालावधीमध्ये दरपत्रके मागविण्यात येत असुन इच्छुक निविदाधारकांनी खालील नमुद पत्त्यावर कार्यालयीन वेळेत सिलबंद लिफाफा मध्ये आपले दरपत्रक सादर करावेत.

सोबत: दरपत्रक नोटीस व विनिर्दिष्टचे जोडली आहेत.

(डॉ.शिल्पा दीमकुंडवार)

अधिष्ठाता,
शासकीय वैद्यकीय महाविद्यालय,
धाराशिव.

प्रत:- १) सुचना फलक जाहीर नोटिस, शासकीय वैद्यकीय महाविद्यालय, धाराशिव.

२) संकेतस्थळ, शासकीय वैद्यकीय महाविद्यालय, धाराशिव.

३) विभागप्रमुख, औषधवैद्यकशास्त्र/स्त्रीरोग व प्रसुतीशास्त्र/
कान-नाक-घसाशास्त्र, शा. वै. म. धाराशिव.

कार्यालयाचा पत्ता

अधिष्ठाता,
शासकीय वैद्यकीय महाविद्यालय,
जिल्हा सामान्य रुग्णालय आवार,
धाराशिव-४१३५०१

दरपत्रक नोटिस

नवनिर्मित शासकीय वैद्यकीय महाविद्यालय व रुग्णालयातील औषधवैद्यकशास्त्र/ स्त्रीरोग व प्रसुतीशास्त्र/ कान-नाक-घसाशास्त्र विभागास रुग्णसेवा व वैद्यकीय अभ्यासक्रमासाठी अत्यावश्यक असलेली यंत्रसामुग्री व साधनसामुग्री खरेदी करून पुरवठा/ प्रस्थापित करणे कामी निविदा धारकाकडून दरपत्रके मागविण्यात येत असून दि. ०९/०९/२०२५ ते दि. १७/०९/२०२५ पर्यंत इच्छुक निविदाधारकांनी अधिष्ठाता, शासकीय वैद्यकीय महाविद्यालय, धाराशिव येथे कार्यालयीन वेळेत सिलबंद लिफाफा मध्ये आपले दरपत्रक करार सादर करावेत.

दरपत्रके सादर करतेवेळी अधिकृत लेटरहेड वर खालील प्रमाणे विहित नमुन्यात तसेच अटी व शर्तीना अनुसरूनच माहिती सादर करावी अन्यथा निविदा प्रक्रियेतून अपात्र करण्यात येईल याची नोंद घ्यावी.

अ.क्र.	यंत्रसामुग्री व साधनसामुग्री	विनिर्दिष्टचे/तपशील	प्रति नग किंमत (सर्व करांसहित) नमुद करावी
औषधवैद्यकशास्त्र/ स्त्रीरोग व प्रसुतीशास्त्र/ कान-नाक-घसाशास्त्र विभाग			
१)	मर्क्युरी बी.पी. ऑपरेटस	विनिर्दिष्टचे सोबत जोडली आहेत	
२)	डिजीटल वेईंग मशिन अडल्ट		
३)	पोर्टेबल सक्शन मशिन		
४)	ई.सी.जी. मशिन		
५)	फिटल डॉपलर		

अटी व शर्ती:

- ०१) दरपत्रक मोहरबंद लिफाफा दिनांक १७/०९/२०२५ पर्यंत सायंकाळी ५.३० वाजेपर्यंत कार्यालयात पोहचतील या बेताने पाठवावेत. जाहिर केलेल्या तारखेनंतर अथवा कार्यालयीन वेळेनंतर आलेले दरपत्रक विचारात घेतले जाणार नाहीत/ ग्राह्य घरले जाणार नाहीत.
- ०२) सुचना फलक/ संकेतस्थळावरील जाहिर नोटीस प्रमाणे इच्छुक कंपनीस दरपत्रक मोहरबंद लिफाफा सादर करण्याची मुभा देण्यात येत आहे. दरपत्रक मोहरबंद लिफाफा "अधिष्ठाता शासकीय वैद्यकीय महाविद्यालय, धाराशिव" यांचे नावे विहित मुदतीत कार्यालयास सादर करावा.
- ०३) दरपत्रक मोहरबंद लिफाफ्यावर "औषधवैद्यकशास्त्र/ स्त्रीरोग व प्रसुतीशास्त्र/ कान-नाक-घसाशास्त्र विभागाची यंत्रसामुग्री व साधनसामुग्री करिता दरपत्रके" तसेच मोहरबंद लिफाफा जमा करण्याचा अंतिम दिनांक दरपत्रधारकाच्या नावाचा शिक्का इत्यादी नमुद असणे आवश्यक आहे.
- ०४) दरपत्रक सिलबंद लिफाफ्यात सादर करावयाचे दस्तऐवज: (Document) जीएसटी (GST) क्रमांक असलेल्या अधिकृत लेटरहेडवर दरपत्रक सादर करावे. त्यासोबत (१) जीएसटी प्राधिकृत प्रत, (२) पॅन कार्ड, (३) शॉप ॲक्ट, (४) शासकीय कार्यालयामध्ये काम केल्याचे मागील तीन (३) वर्षांचे अनुभव प्रमाणपत्र (Valid PO), (०५) आयकर परतावा (२०२१-२२, २०२२-२३, २०२३-२४) इत्यादी प्रमाणपत्रांची स्वाक्षांकित छायांकित प्रत (५) प्रात्यक्षिक अहवाल (सोबत नमुना जोडला आहे) "ANNEXURE-A" (६) स्थळ पाहणी अहवाल (Site Visit Report-सोबत नमुना जोडला आहे) "ANNEXURE-B" (७) एकल दरपत्रक धारक असल्याबाबतचे हमीपत्र (सोबत नमुना जोडला आहे) "ANNEXURE-C" व (८) अनामत रकमेचा मुळ घनाकर्ष इ. सर्व दस्तऐवज जोडणे बंधनकारक आहे.
- ०५) निविदा/दरपत्रके सादर करणाऱ्या उमेदवाराने "अधिष्ठाता, शासकीय वैद्यकीय महाविद्यालय, धाराशिव" यांचे नावे स्टेट बँक ऑफ इंडिया, जिल्हा न्यायालय शाखा, धाराशिव येथे देय रु.३५,०००/- एवढ्या अनामत रकमेचा डिमांड ड्राफ्ट दरपत्रक लिफाफ्यामध्ये सादर करणे बंधनकारक आहे.
- ०६) निविदा सादर करण्याच्या अंतिम दिनांकापुर्वी निविदेतील नमुद साहित्याचे विनिर्दिष्ट्यानुसार (Specifications) खरेदी समिती/ वापरकर्ता विभागास प्रात्यक्षिक (Demo) दाखवून त्याचा अहवाल दरपत्रकामध्ये जोडून सादर करणे बंधनकारक आहे. अन्यथा निविदा प्रक्रियेतून अपात्र करण्यांत येईल.
- ०७) निविदा सादर करण्याच्या अंतिम दिनांकापुर्वी स्थळ पाहणी (Site Visit) करून तसा अहवाल दरपत्रकामध्ये जोडून सादर करण्यात यावा.

०८) पूरवठाधारकास आगाऊ रक्कम (ADVANCE PAYMENT) अदा करण्यात येणार नाही. अपवादात्मक परिस्थितीमुळे देयक अदा करण्यास झालेल्या विलंबापोटी कोणत्याही स्वरुपाचे व्याज अथवा अतिरिक्त शुल्क/ रक्कम हे कार्यालय अदा करणार नाही. तसेच अशा प्रकारची कोणतीही मागणी मान्य करता येणार नाही.

०९) सर्वात कमी दर सादर करणाऱ्या पात्र निविदाधारकाचे दर हे पूढिल ०६ महिन्यांकरिता गोठविण्यांत येतील. कार्यालयाच्या आवश्यकतेनुसार वेळोवेळी त्याच दराने सामुग्री विहित वेळेत पूरवठा करणे बंधनकारक राहिल.

१०) निविदा घोषित झाल्यानंतर निविदाधारक यांनी निविदेतील यंत्रे/उपकरणे इत्यादी साहित्याच्या बाबतीत विनिर्दिष्ट्यामध्ये नमुद केल्यानुसार सदर यंत्राचा/ उपकरणांचा वॉरंटी कालावधी, सर्वसमावेशक देखभाल करार (CMC), वार्षिक देखभाल करार (AMC) इत्यादी बाबत रु.५०० (अक्षरी: पाचशे रुपये मात्र) इतक्या रमेच्या बॉडवर हमीपत्र (नोटरी करुन) कार्यालयात सादर करणे बंधनकारक आहे. तदनंतरच पूरवठा करण्यात आलेल्या साहित्याची देयके अदा करण्यात येतील.

Warranty /CMC (Comprehensive maintenance contract)

- A. वॉरंटी विनिर्दिष्ट्यामध्ये नमुद केलेल्या कालावधीसाठी वैध राहिल. तदनंतर शासनाने विहित केलेल्या दरानुसार सी.एम.सी./ए.एम.सी. सेवा पुरविण्यात येईल.
- B. वॉरंटी/सीएमसी कालावधीमध्ये तपासणी सेवा मोफत दिली जावी.
- C. वॉरंटी कालावधीमध्ये कोणत्याही प्रकारच्या दुरुस्ती सेवेसाठी कोणतेही सेवा शुल्क लागू नाही.
- D. वॉरंटी/सीएमसी कालावधीमध्ये यंत्राच्या/उपकरणाच्या स्थितीच्या प्रत्येक तक्रारीवर जास्तीत जास्त ०३ दिवसांच्या आत तातडीने उपाययोजना केली जाईल.

११) सदरील निविदाप्रक्रियेमध्ये नमुद यंत्रसामुग्री व साधनसामुग्री करिता एक पेक्षा जास्त न्युनतम दरधारक (Item wise) प्राप्त झाले असता एकत्रित किंमत मुल्यांकन (Total Value wise Evaluation) पध्दतीने सर्वात न्युनतम दर सादर करणाऱ्या निविदाधारकास पूरवठा आदेश देण्यात येतील.

१२) वरील सर्व अटी व शर्ती मान्य असल्याबाबत अधिकृत लेटरहेडवर सही व शिक्क्यासह शपथपत्र/हमीपत्र दरपत्रकासोबत दाखल करणे बंधनकारक आहे. अन्यथा निविदा प्रक्रियेतुन अपात्र करण्यात येईल याची नोंद घ्यावी.

१३) अपवादात्क परिस्थितीमुळे उक्त कोणत्याही अटी अथवा शर्तीमध्ये आवश्यकतेनुसार अंशतः बदल करणे अथवा प्राप्त झालेली दरपत्रके कोणतेही कारण/पुर्वसुचना न देता नाकारणे तसेच कोणत्याही स्तरावर निविदा प्रक्रिया रद्द करणे इ. अधिकार संस्थाप्रमुख (अधिष्ठाता) यांनी राखुन ठेवलेले आहेत.

नोंद:- सदर दर पत्रके मा.अधिष्ठाता यांचे दालनात उघडण्याची वेळ दिनांक. 20/09/2024 रोजी ११.३० वाजता राहिल. नियोजित वेळेत कोणताही बदल झाल्यास निविदाधारकांना तशी पुर्वसुचना देण्यात येईल.

(डॉ.शिल्पा दीमकुंडवार)

अधिष्ठाता,

शासकीय वैद्यकीय महाविद्यालय,

धाराशिव.

**Technical Compliance Chart/ Demo Report
(On Bidder Letters Head)**

**To,
The Dean,
Government Medical College,
Dharashiv**

**Subject: About Submission of Technical Compliance Chart/ Demonstration Reprot.
Reference: Your Tender/Quotation No & Date:**

Sr No.	Name of Instrument as asked in the tender form	Quoted Instrument details by the tenderer	Whether the tender quoted by the supplier is as per specification asked for Indicate against each item clearly YES/NO

**User/ Head Of Department
Government Medical College,
Dharashiv**

**User/ Head Of Department
Government Medical College,
Dharashiv**

**Signature with Stamp & Seal
OEM/ Othorised Dealer**

/ /2025

To
The Dean,
Government Medical Collage,
Dharashiv-413501

Sub: About subbmission of Site Visit Report.

Ref: Bid/Tender/Quotation Number:

Bidder Name :

Our Engineer/ Office Person have Visited the Site Mentioned Below in Consideration and Have understand All technical Details and local condition prevailing for Finishing. The wok and ready to complete the supply, Installation and training work (as applicable).

GPS Photo of site visited Engineer with Government Medical collage employee provided by collage.

**User/ Head Of Department
Government Medical College,
Dharashiv**

**User/ Head Of Department
Government Medical College,
Dharashiv**

**Signature with Stamp & Seal
OEM/ Othorised Dealer**

एकल दरपत्रक अधिकृत विक्रेता/पुरवठादार/कंपनी यांचे लेटरहेड

Letter No.

Date :-

प्रति
अधिष्ठाता,
शासकीय वैद्यकीय महाविद्यालय,
धाराशिव.

विषय :- एकल दरपत्रक सादर करणेसंबंधीचे हमीपत्र सादर करणेबाबत...

संदर्भ :- आपले दरपत्रक मागणी पत्र

क्रमांक. _____

दिनांक _____

महोदय

संदर्भाकित दरपत्रक मागणी पत्रानुसार मागणी करण्यात आलेले एकल दरपत्रक सादर करण्यासंबंधीचे हमीपत्र मी खालील प्रमाणे सादर करित आहे.

हमीपत्र (Undertaking)

याद्वारे हमी देतो की, दरपत्रक प्रक्रियेसाठी एकच दरपत्रक सादर करित आहे. आमच्याच फर्मशी निगडित असलेल्या कुठल्याही व्यक्तीच्या नावे किंवा अप्रत्यक्षपणे केवळ आम्हास लाभ होईल, अश्याप्रकारे दुसरे दरपत्रक दरपत्रकप्रक्रियेमध्ये सादर केलेला नाही. तसेच माझा/आमचा आपल्या कार्यालयातील खरेदी प्राधिकार्यांशी कुठलेही हितसंबंध नाही.

उक्त बाब भविष्यात असत्य/खोटी आढळून आल्यास, सर्वस्वी जबाबदारी आमची राहिल. नियमानुसार होणाऱ्या कार्यवाहीस मी/आम्ही पात्र असू. तदसंबंधी माझी/आमची कुठलीही हरकत राहणार नाही. अशी याद्वारे हमी देत आहे.

अधिकृत व्यक्तिके नाव व स्वाक्षरी,
शिक्का आणि मोहर
Authorized Person Name,
Signature
with Stamp and Seal

**General Medicine/ OBGY/ ENT Department
Technical Specifications**

Water Cooler S.S.

- **High Capacity:** The water cooler provides a substantial cooling capacity of 40 liters per hour and a storage capacity of 80 liters, making it a suitable choice for larger groups.
- **Double Tap System:** This water cooler features two taps, ensuring a continuous supply of refreshing cold water for numerous people at once.
- **Sturdy Construction:** The entire body of the cooler is crafted from stainless steel, promising durability, corrosion resistance, and ease of cleaning.
- **Efficient Cooling Mechanism:** Equipped with a hermetically sealed, reciprocating compressor and R 134s refrigerant for reliable and consistent cooling performance.
- **Perfect for Larger Groups:** Capable of catering to 80-100 individuals and serving up to 200 glasses per hour, it's ideal for offices, schools, or community centers.
- **Made in India:** The water cooler is a product of Indian design and manufacturing, ensuring excellent quality and service standards.

Stethoscope

The stethoscope is a medical device for auscultation, or listening to internal sounds of an animal or human body. It typically has a small disc-shaped resonator that is placed against the skin, with either one or two tubes connected to two earpieces.

Mercury BP Apparatus

- **Accurate Blood Pressure Monitoring:** Utilizes mercury for precise and reliable blood pressure measurements, ensuring accuracy in both professional and personal settings.
- **Professional Grade Precision:** Designed to meet the standards of healthcare professionals, delivering consistent and trustworthy readings with each use.
- **Suitable for Personal Use:** Ideal for individuals monitoring their blood pressure at home, offering convenience and reliability for personal health management.
- **Durable Construction:** Constructed with high-quality materials for durability and longevity, providing reliable performance over time.

Laryngoscope Adult

- **Comprehensive Laryngoscope Set:** is specifically designed for adult use, featuring the versatile Macintosh type blades. The set includes four blade sizes: 1, 2, 3, and 4, to accommodate a wide range of anatomical variations and medical needs.
- **High-Quality Stainless Steel Construction:** Both the handle and blades of this laryngoscope set are made from 304-grade stainless steel, ensuring durability and longevity. The stainless steel construction also provides ease of sterilization and maintenance.
- **Efficient LED Illumination:** Equipped with a removable LED lamp, this laryngoscope set offers bright and clear visibility, which is crucial for precise medical examinations and procedures. The LED technology ensures efficient energy use and consistent light output.
- **Durable Finish and Accessories:** The set boasts a dull/matt finish, reducing glare and enhancing visual comfort during use. It comes supplied with two batteries for the handle, ensuring that the laryngoscope is always ready for use. Additionally, one spare LED lamp and batteries are provided for convenience.
- **Versatile and Reliable:** Designed to cater to various medical situations, this laryngoscope set adult 4 blade is a reliable choice for healthcare professionals. Its versatility, combined with the quality of materials and construction, makes it a valuable tool in any medical setting.

Laryngoscope Pediatric

- **Premium Quality Construction:** Laryngoscope Set boasts high-grade 304 stainless steel blades and handles, guaranteeing durable, reliable performance and longevity. Each set comes with a reassuring two-year warranty, highlighting its superior standard and quality.
- **Advanced Illumination Technology:** Each blade in the set is equipped with cool LED bulbs, ensuring bright, clear illumination while eliminating the risk of accidental burns to patients' delicate tissues. These LED bulbs are not only three times brighter but also enjoy a tenfold increase in battery life compared to traditional alternatives.
- **Versatile Design & Compatibility:** With blades available in both Macintosh and Miller types, the set offers versatility in use. Each blade is meticulously designed with a brushed satin finish to minimize glare and is

From:

Adhikari

- compatible with all conventional handles. The blades also come in a range of sizes (from 00 to 5), making the set suitable for various patient needs.
- **Safety-Focused Features:** Prioritizing patient safety and comfort, the laryngoscope blades are crafted with atraumatic tips. This thoughtful design feature minimizes discomfort and potential trauma during intubation, making the procedure smoother and safer for patients.
 - **ISO-Compliant Handles:** Conforming to ISO 7376(1), the handles in this set fit standard blades, featuring a knurled surface for a secure grip. This thoughtful design supports confident and efficient use by medical professionals during procedures. Manufactured by IndoSurgicals, a trusted name in health, these handles embody commitment to quality and innovation, designed to support and enhance patient care while meeting the rigorous demands of healthcare environments effectively.

Knee Hammer

Knee hammer is a medical instrument that is used by doctors and medical practitioners to test deep tendon reflexes. Testing for reflexes is one of the most important diagnosing tests of neurological diseases in order to detect abnormalities in the central or peripheral nervous system.

Slide Stand

- Slide holder with inclined channels for cleaning and drying microscope slides
- Holds 1 x 3" and 2 x 3" microscope slides (sold separately)
- Polyethylene construction for durability and chemical resistance
- Assorted sizes hold up to 15, 40, or 78 slides

Refrigerator

Efficient and Energy-saving fridge-freezer-combination. Color: White. Finish: Semi-glossy. No frost technology. Net Weight: 46 kg. Gross Weight: 50 kg. Dimensions: 54.5 x 59.5 x 141.7 cm. Package Dimensions: 57.5 x 62.2 x 146.2 cm. Annual Energy Consumption: 404 KWh/ Year. Fridge Volume in Liter: 144. Freezer Volume in Liter: 53. ESMA 3 Star Rating. Power: 220-240V, frequency 50Hz. Home-use & professional-use. High storage-volume with drawer and box. One year warranty.

Digital Weighing Machine Adult

- Easy-to-read lcd display, digit size: 36 mm
- Xl size: 32 x 30.5 cm
- Standing surface made from extra strong 8 mm safety glass. Change over to kg/lb/system
- Capacity: 180 kg, graduation: 100 g, overload indication, automatic switch-on/ switch-off
- Incl. 2 x 3V cr2032 battery

Digital Weighing Machine Pediatric

- Easy-to-read lcd display, digit size: 36 mm
- Xl size: 32 x 30.5 cm
- Standing surface made from extra strong 8 mm safety glass. Change over to kg/lb/system
- Capacity: 100 kg, graduation: 100 g, overload indication, automatic switch-on/ switch-off
- Incl. 2 x 3V cr2032 battery

Digital Weighing Machine Neonatal

- Accurate and reliable digital baby weighing scale
- Suitable for newborns and infants up to 30kg capacity
- Secure and comfortable tray for baby's safety during weighing
- Easy-to-read digital display for convenient monitoring
- Compact design for home or travel use

Portable Suction Machine

Should be designed for draining blood and other fragmetic secrtetions in operation room and emergency room in hospital.

Should be fitted with oil immersed noiseless motorized vacuum pump.

Cabinet made from stainless steel.

[Handwritten Signature]

[Handwritten Signature]

Two glass jars on the top of having minimum capacity of 2 Ltrs fitted with rubber air tight lids and overflow safety device.
Should be supplied with adequately long pressure tubing providing required pressure.
Should have vacuum control by knob.
Should be mounted on four caster wheels.
Should have motor of 1/4 HP capacity and power consumption not more than 250 Watts.
Should have vacuum at least between 100 mm Hg to at least 575 mm Hg (-75 kPa).
International standards: the unit should comply with international standards and should have CE or FDA marking.

ECG Machine


- 7" TFT, touch screen, led backlight
- Digital isolation technology and signal processing solution, digital filter
- Patient management, name and age and id.
- Detail analysis report.
- Multi-language options: German, French, Italian, Turkish
- Built-in lithium rechargeable battery, wide thermal printing system
- USB and LAN socket.
- Memory: Built-in memory or mini SD Memory card. Store and archive more than 1000 readings.
- Auto-measurement, auto-analysis, and auto-interpretation.
- Patient leak current: <math><10\mu A</math>
- Input impedance: $\geq 50 \Omega$
- Frequency response: $0.05 \sim 150\text{HZ}(-3\text{dB})$
- Time constant: $>3.2\text{S}$
- CMRR: $>100\text{dB}$
- Dimension of recording paper: 80mmx20m
- Paper speed: 25mm/s, 50mm/s
- Sensitivity choice: 5, 10, 20mm/mV.
- Measurement parameters: HR, P-R interval, P-Duration, QRS Duration, Q-T interval, QTc, P Axis, QRS Axis, T Axis, R(V5), S(V1), R(V5)+S(V1)
- Product safety type: Class I, CF. Defibrillation and pacing protection

Fetal Doppler


- Portable Design, LCD Display with white backlight
- Accurate and reliable FHR detection
- Highly sensitive probe with DSP technology
- Frequency 2.0Mhz in continuous wave
- Dimensions : 330x230x70mm
- Weight : 1 kg

FHR:


- Measurement range : 30BPM - 240BPM
- Accuracy : $\pm 1\%$ or $\pm 1\text{BPM}$

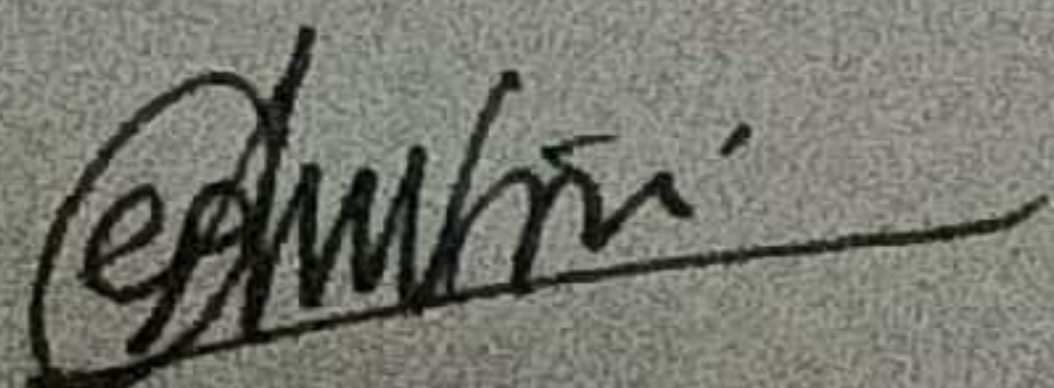

(Dr. Ashvini Somware)
Assistant Professor
Dept. of ENT
Government Medical College
Dharashiv

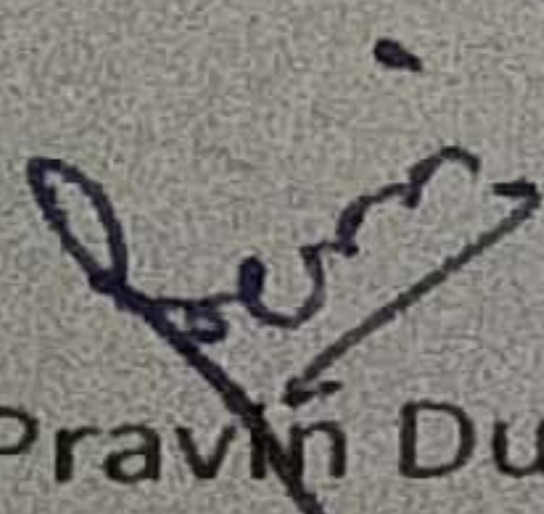

(Dr. Pravin Dumane)
Assistant Professor
Dept. of General Medicine
Government Medical College
Dharashiv

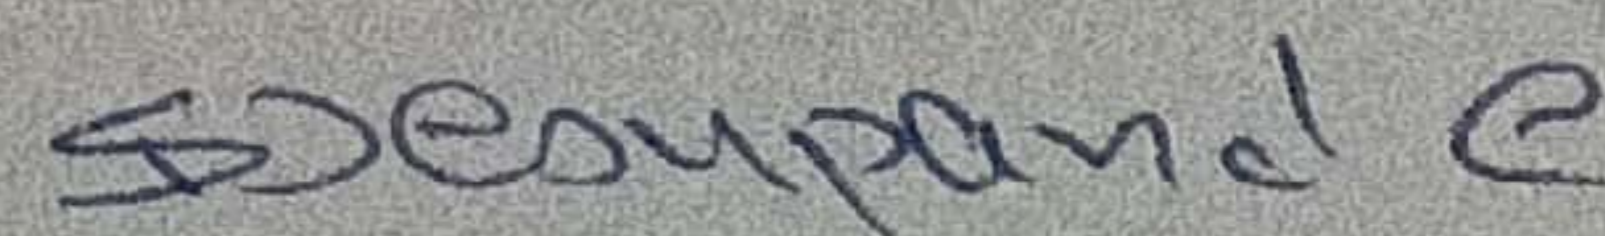

(Dr. Sonali Deshpande)
Associate Professor & Head
Dept. of OBGY
Government Medical College
Dharashiv