
	<p style="text-align: center;">महाराष्ट्र शासन शासकीय वैद्यकीय महाविद्यालय, धाराशिव GOVERNMENT MEDICAL COLLEGE, DHARASHIV कोविड-१९ इमारत, जिल्हा रुग्णालय आवार, धाराशिव. (महाराष्ट्र) 413 501 e-mail: deangmcosmanabad@gmail.com</p>	
<p>जा.क्र./शावैमघा/भांडार/रा.यो./दरपत्रके/ 109 /२०२५</p>		<p>दिनांक: 09 /०९/२०२५</p>

प्रति,

-----  
-----  
-----

विषय :- सन २०२४-२५ या वित्तीय वर्षाकरिता राज्य योजना (स्टेट-प्लॅन) अंतर्गत प्रदान करण्यात आलेल्या प्रशासकीय मान्यते मधील यंत्रसामुग्री व साधनसामुग्री खरेदीकरिता दरपत्रके प्रसिध्द करणेबाबत.  
संदर्भ :- दिनांक ०६ /०९/२०२५ रोजीची मंजुर कार्यालयीन टिप्पणी.

उपरोक्त विषयास अनुसरुन कळविण्यात येते की नवनिर्मित शासकीय वैद्यकीय महाविद्यालय, धाराशिव या संस्थेतील कान-नाक-घसाशास्त्र विभागास वैद्यकीय अभ्यासक्रम व रुग्णसेवेकरिता विविध यंत्रसामुग्री व साधनसामुग्री खरेदी करण्याची संस्थेस आवश्यकता आहे.

तरी मागणीप्रमाणे उच्च दर्जाची यंत्रसामुग्री व साधनसामुग्री खरेदी करुन पुरवठा/प्रस्थापित करणेकामी पात्र निविदा धारकांकडुन विहित अटी व शर्तीना अनुसरुन दि.२९ /०९ /२०२५ ते दि.१७ /११ /२०२५ कालावधीमध्ये दरपत्रके मागविण्यात येत असुन इच्छुक निविदाधारकांनी खालील नमुद पत्त्यावर कार्यालयीन वेळेत सिलबंद लिफाफा मध्ये आपले दरपत्रक सादर करावेत.

सोबत: दरपत्रक नोटीस व विनिर्दिष्टचे जोडली आहेत.



(डॉ.शिल्पा दोमकुंडवार)  
अधिष्ठाता,  
शासकीय वैद्यकीय महाविद्यालय,  
धाराशिव.

- प्रत:- १) सुचना फलक जाहीर नोटिस, शासकीय वैद्यकीय महाविद्यालय, धाराशिव.  
२) संकेतस्थळ, शासकीय वैद्यकीय महाविद्यालय, धाराशिव.  
३) विभाग प्रमुख, कान-नाक-घसा शास्त्र, शा.वै.म., धाराशिव.

कार्यालयाचा पत्ता  
  
अधिष्ठाता,  
शासकीय वैद्यकीय महाविद्यालय,  
जिल्हा सामान्य रुग्णालय आवार,  
धाराशिव-४१३५०९



दरपत्रक नोटिस

नवनिर्मित शासकीय वैद्यकीय महाविद्यालय व रुग्णालयातील कान-नाक-घसाशास्त्र विभागास रुग्णसेवा व वैद्यकीय अभ्यासक्रमासाठी अत्यावश्यक असलेली यंत्रसामुग्री व साधनसामुग्री खरेदी करून पुरवठा/ प्रस्थापित करणे कामी निविदा धारकाकडून दरपत्रके मागविण्यात येत असून दि. ०९/०१/२०२५ ते दि. १७/०१/२०२५ पर्यंत इच्छुक निविदाधारकांनी अधिष्ठाता, शासकीय वैद्यकीय महाविद्यालय, धाराशिव येथे कार्यालयीन वेळेत सिलबंद लिफाफा मध्ये आपले दरपत्रक करार सादर करावेत.

दरपत्रके सादर करतेवेळी अधिकृत लेटरहेड वर खालील प्रमाणे विहित नमुन्यात तसेच अटी व शर्तीना अनुसरूनच माहिती सादर करावी अन्यथा निविदा प्रक्रियेतून अपात्र करण्यात येईल याची नोंद घ्यावी.

अ.क्र.	यंत्रसामुग्री व साधनसामुग्री	विनिर्दिष्टचे/तपशील	प्रति नग किंमत (सर्व करांसहित) नमुद करावी
<b>कान-नाक-घसाशास्त्र विभाग</b>			
१)	स्टरलायझर	विनिर्दिष्टचे सोबत जोडली आहेत	
२)	सायडेक्स इस्टुमेंट		
३)	बी.पी.एॅपरॅटस		
४)	स्टेथोस्कोप		
५)	नेझल स्पेक्युलम डिफ्रॅन्ट साईजेस		
६)	लॅक्स टंग डिप्रेसर डिफ्रॅन्ट साईजेस		
७)	लॅरिंगल मिरर डिफ्रॅन्ट साईजेस		
८)	नॅसोफेरिंगल मिरर डिफ्रॅन्ट साईजेस		
९)	औरल स्पेक्युलम डिफ्रॅन्ट साईजेस		
१०)	इअर सक्शन डिफ्रॅन्ट साईजेस		
११)	नेझल सक्शन डिफ्रॅन्ट साईजेस		
१२)	सक्शन अॅपरॅटस		
१३)	सिगल्स स्पेक्युलम		
१४)	टयुनिंग फोर्क (५१२ Hz)		
१५)	टयुनिंग फोर्क (२५६ Hz)		
१६)	टयुनिंग फोर्क (१०२४ Hz)		
१७)	एॅटोस्कोप विथ हॅलोजन बल्ब, रिचार्जबल बॅटरी, अॅण्ड सिगल अॅटॅचमेंट		
१८)	बायोनेट फोरसेप्स		
१९)	बुल्स लॅम्प		
२०)	हेड मिरर		
२१)	हेड लाईट विथ एल.ई.डी/ हॅलोजन लॅम्प		
२२)	जॉबसन हॉर्न प्रोब		
२३)	इन्स्ट्रुमेंट ट्रे		
२४)	किडनी ट्रे		

अटी व शर्ती:

- ०१) दरपत्रक मोहरबंद लिफाफा दिनांक १७/०१/२०२५ पर्यंत सायंकाळी ५.३० वाजेपर्यंत कार्यालयात पोहचतील या बेताने पाठवावेत. जाहिर केलेल्या तारखेनंतर अथवा कार्यालयीन वेळेनंतर आलेले दरपत्रक विचारात घेतले जाणार नाहीत/ ग्राह्य घरले जाणार नाहीत.
- ०२) सुचना फलक/ संकेतस्थळावरील जाहिर नोटीस प्रमाणे इच्छुक कंपनीस दरपत्रक मोहरबंद लिफाफा सादर करण्याची मुभा देण्यात येत आहे. दरपत्रक मोहरबंद लिफाफा "अधिष्ठाता शासकीय वैद्यकीय महाविद्यालय, धाराशिव" यांचे नावे विहित मुदतीत कार्यालयास सादर करावा.
- ०३) दरपत्रक मोहरबंद लिफाफ्यावर "कान-नाक-घसाशास्त्र विभागाची यंत्रसामुग्री व साधनसामुग्री करिता दरपत्रके" तसेच मोहरबंद लिफाफा जमा करण्याचा अंतिम दिनांक दरपत्रधारकाच्या नावाचा शिक्का इत्यादी नमुद असणे आवश्यक आहे.



- ०४) दरपत्रक सिलबंद लिफाफ्यात सादर करावयाचे दस्तऐवज: (Document) जीएसटी (GST) क्रमांक असलेल्या अधिकृत लेटरहेडवर दरपत्रक सादर करावे. त्यासोबत (१) जीएसटी प्राधिकृत प्रत, (२) पॅन कार्ड, (३) शॉप ॲक्ट, (४) शासकीय कार्यालयामध्ये काम केल्याचे मागील तीन (३) वर्षांचे अनुभव प्रमाणपत्र (Valid PO), (०५) आयकर परतावा (२०२१-२२, २०२२-२३, २०२३-२४) इत्यादी प्रमाणपत्रांची स्वाक्षांकित छायांकित प्रत (५) प्रात्यक्षिक अहवाल (सोबत नमुना जोडला आहे) "ANNEXURE-A" (६) स्थळ पाहणी अहवाल (Site Visit Report-सोबत नमुना जोडला आहे) "ANNEXURE-B" (७) एकल दरपत्रक धारक असल्याबाबतचे हमीपत्र (सोबत नमुना जोडला आहे) "ANNEXURE-C" व (८) अन्नामत रकमेचा मुळ धनाकर्ष इ. सर्व दस्तऐवज जोडणे बंधनकारक आहे.
- ०५) निविदा सादर करण्याच्या अंतिम दिनांकापुर्वी निविदेतील नमुद साहित्याचे विनिर्दिष्ट्यानुसार (Specifications) खरेदी समिती/ वापरकर्ता विभागास प्रात्यक्षिक (Demo) दाखवुन त्याचा अहवाल दरपत्रकामध्ये जोडुन सादर करणे बंधनकारक आहे. अन्यथा निविदा प्रक्रियेतून अपात्र करण्यांत येईल.
- ०६) निविदा सादर करण्याच्या अंतिम दिनांकापुर्वी स्थळ पाहणी (Site Visit) करुन तसा अहवाल दरपत्रकामध्ये जोडुन सादर करण्यात यावा.
- ०७) पुरवठाधारकास आगाऊ रक्कम (ADVANCE PAYMENT) अदा करण्यात येणार नाही. अपवादात्मक परिस्थितीमुळे देयक अदा करण्यास झालेल्या विलंबापोटी कोणत्याही स्वरुपाचे व्याज अथवा अतिरिक्त शुल्क/ रक्कम हे कार्यालय अदा करणार नाही. तसेच अशा प्रकारची कोणतीही मागणी मान्य करता येणार नाही.
- ०८) सर्वात कमी दर सादर करणाऱ्या पात्र निविदाधारकाचे दर हे पूढिल ०६ महिन्यांकरिता गोठविण्यांत येतील. कार्यालयाच्या आवश्यकतेनुसार वेळोवेळी त्याच दराने सामुग्री विहित वेळेत पुरवठा करणे बंधनकारक राहिल.
- ०९) निविदा घोषित झाल्यानंतर निविदाधारक यांनी निविदेतील यंत्रे/उपकरणे इत्यादी साहित्याच्या बाबतीत विनिर्दिष्ट्यामध्ये नमुद केल्यानुसार सदर यंत्राचा/ उपकरणांचा वॉरंटी कालावधी, सर्वसमावेशक देखभाल करार (CMC), वार्षिक देखभाल करार (AMC) इत्यादी बाबत रु.५०० (अक्षरी: पाचशे रुपये मात्र) इतक्या रमेच्या बाँडवर हमीपत्र (नोटरी करुन) कार्यालयात सादर करणे बंधनकारक आहे. तदनंतरच पुरवठा करण्यात आलेल्या साहित्याची देयके अदा करण्यात येतील.

**Warranty /CMC (Comprehensive maintenance contract)**

- A. वॉरंटी विनिर्दिष्ट्यामध्ये नमुद केलेल्या कालावधीसाठी वैध राहिल. तदनंतर शासनाने विहित केलेल्या दरानुसार सी.एम.सी./ए.एम.सी. सेवा पुरविण्यात येईल.
- B. वॉरंटी/सीएमसी कालावधीमध्ये तपासणी सेवा मोफत दिली जावी.
- C. वॉरंटी कालावधीमध्ये कोणत्याही प्रकारच्या दुरुस्ती सेवेसाठी कोणतेही सेवा शुल्क लागू नाही.
- D. वॉरंटी/सीएमसी कालावधीमध्ये यंत्राच्या/उपकरणाच्या स्थितीच्या प्रत्येक तक्रारीवर जास्तीत जास्त ०३ दिवसांच्या आत तातडीने उपाययोजना केली जाईल.
- १०) सदरील निविदाप्रक्रियेमध्ये नमुद यंत्रसामुग्री व साधनसामुग्री करिता एक पेक्षा जास्त न्युनतम दरधारक (Item wise) प्राप्त झाले असता एकत्रित किंमत मुल्यांकन (Total Value wise Evaluation) पध्दतीने सर्वात न्युनतम दर सादर करणाऱ्या निविदाधारकास पुरवठा आदेश देण्यात येतील.
- ११) वरील सर्व अटी व शर्ती मान्य असल्याबाबत अधिकृत लेटरहेडवर सही व शिक्क्यासह शपथपत्र/हमीपत्र दरपत्रकासोबत दाखल करणे बंधनकारक आहे. अन्यथा निविदा प्रक्रियेतून अपात्र करण्यात येईल याची नोंद घ्यावी.
- १२) अपवादात्क परिस्थितीमुळे उक्त कोणत्याही अटी अथवा शर्तीमध्ये आवश्यकतेनुसार अंशतः बदल करणे अथवा प्राप्त झालेली दरपत्रके कोणतेही कारण/पुर्वसुचना न देता नाकारणे तसेच कोणत्याही स्तरावर निविदा प्रक्रिया रद्द करणे इ. अधिकार संस्थाप्रमुख (अधिष्ठाता) यांनी राखुन ठेवलेले आहेत.
- नोंद:- सदर दर पत्रके मा.अधिष्ठाता यांचे दालनात उघडण्याची वेळ दिनांक. 20/09/2024 रोजी ११.३० वाजता राहिल. नियोजित वेळेत कोणताही बदल झाल्यास निविदाधारकांना तशी पुर्वसुचना देण्यात येईल.

(डॉ.शिल्पा दोमकुंडवार)

अधिष्ठाता,  
शासकीय वैद्यकीय महाविद्यालय,  
धाराशिव.



**ANNEXURE-A**

**Technical Compliance Chart/ Demo Report  
(On Bidder Letters Head)**

To,  
The Dean,  
Government Medical College,  
Dharashiv

**Subject: About Submission of Technical Compliance Chart/ Demonstration Reprot.  
Reference: Your Tender/Quotation No & Date:**

Sr No.	Name of Instrument as asked in the tender form	Quoted Instrument details by the tenderer	Whether the tender quoted by the supplier is as per specification asked for Indicate against each item clearly YES/NO

User/ Head Of Department  
Government Medical College,  
Dharashiv

User/ Head Of Department  
Government Medical College,  
Dharashiv

Signature with Stamp & Seal  
OEM/ Othorised Dealer



/ /2025

To  
The Dean,  
Government Medical Collage,  
Dharashiv-413501

**Sub: About subbmission of Site Visit Report.**

**Ref: Bid/Tender/Quotation Number:**

**Bidder Name :**

Our Engineer/ Office Person have Visited the Site Mentioned Below in Consideration and Have understand All technical Details and local condition prevailing for Finishing. The wok and ready to complete the supply, Installation and training work (as applicable).

GPS Photo of site visited Engineer with Government Medical collage employee provided by collage.

User/ Head Of Department  
Government Medical College,  
Dharashiv

User/ Head Of Department  
Government Medical College,  
Dharashiv

Signature with Stamp & Seal  
OEM/ Othorised Dealer



एकल दरपत्रक अधिकृत विक्रेता/पुरवठादार/कंपनी यांचे लेटरहेड

Letter No.

Date :-

प्रति  
अधिष्ठाता,  
शासकीय वैद्यकीय महाविद्यालय,  
धाराशिव.

विषय :- एकल दरपत्रक सादर करणेसंबंधीचे हमीपत्र सादर करणेबाबत...

संदर्भ :- आपले दरपत्रक मागणी पत्र

क्रमांक. \_\_\_\_\_

दिनांक \_\_\_\_\_

महोदय

संदर्भाकित दरपत्रक मागणी पत्रानुसार मागणी करण्यात आलेले एकल दरपत्रक सादर करण्यासंबंधीचे हमीपत्र मी खालील प्रमाणे सादर करित आहे.

**हमीपत्र (Undertaking)**

याद्वारे हमी देतो की, दरपत्रक प्रक्रियेसाठी एकच दरपत्रक सादर करित आहे. आमच्याच फर्मशी निगडीत असलेल्या कुठल्याही व्यक्तीच्या नावे किंवा अप्रत्यक्षपणे केवळ आम्हास लाभ होईल, अश्याप्रकारे दुसरे दरपत्रक दरपत्रकप्रक्रियेमध्ये सादर केलेला नाही. तसेच माझा/आमचा आपल्या कार्यालयातील खरेदी प्राधिकार्यांशी कुठलेही हितसंबंध नाही.

उक्त बाब भविष्यात असत्य/खोटी आढळुन आल्यास, सर्वस्वी जबाबदारी आमची राहिल. नियमानुसार होणाऱ्या कार्यवाहीस मी/आम्ही पात्र असू. तद्संबंधी माझी/आमची कुठलीही हरकत राहणार नाही. अशी याद्वारे हमी देत आहे.

अधिकृत व्यक्तीचे नाव व स्वाक्षरी,  
शिक्का आणि मोहर  
Authorized Person Name,  
Signature  
with Stamp and Seal



## Department of ENT Technical Specifications

### Sterilizer

#### Specification

- An electric instrument sterilizer is a type of sterilizer that uses electricity to generate heat and sterilize medical instruments, tools, and other equipment.
- Electric instrument sterilizers work by heating the instruments to a high temperature for a certain amount of time to kill all microorganisms present on the surface of the instruments.
- The sterilization process typically takes between 30 to 60 minutes, depending on the model of the sterilizer.
- Regular maintenance and cleaning of the sterilizer are also necessary to ensure optimal performance and prolong the lifespan of the equipment.
- Electric instrument sterilizer 14INCH 220-240 Volts, single phase Comes with Sterilization Boxes, Power Code, Tray and Tray Lifting arrangement.

### Cidex Instrument Tray

#### Specification

- Stainless Steel Tray with Cover
- Cidex tray Size approx 27"x6"x5" inches
- Supplied with Inner Perforated Tray with Side handle
- Cidex trays are used to accommodate Medical Instruments and Endoscopes. Stainless Steel Cidex Tray is durable and Reusable.

### BP Apparatus

#### Specification

- Hypertension Indicator
- Intelli Sense Technology. Minimum Pressure Measurement Range 0 mmHg. Maximum Pressure Measurement Range 299 mmHg
- Easy one touch Operations
- Large Display screen
- Memory for Last reading

*[Handwritten signature]*



## Stethoscope

### Specification

- Lightest weight of all Littmann adult stethoscopes at just 118 grams
- Dual-sided chestpiece provides versatility of both a tunable diaphragm and open bell
- Teardrop-shaped chestpiece for easier positioning under blood pressure cuffs and around bandages
- Tunable diaphragm: Hear high or low frequency sounds by slightly adjusting pressure on the chestpiece
- Soft-sealing eartips provide an excellent acoustic seal and comfortable fit
- Two Year warranty
- Used as a diagnostic aid as part of the physical assessment of a patient

## Thudicum/St.Clair Thomson Nasal Speculum different sizes

### Specification

Material	Stainless Steel
Usage/Application	Hospital, Clinical
Size/Dimension	80 mm L
Color	Silver
Surface Finish	Polished

## Lac's Tongue depressor different sizes

### Specification

- Stainless steel tongue depressor
- Made from non magnetizing stainless steel
- L- shape Set of 3 pcs. -
- size 1, 2 and 3

Adhish



## **Laryngeal mirrors different sizes**

### **Specifications**

There are optional types with different mirror diameters of 10mm, 12mm, 14mm, 16mm, 18mm, 20mm, 22mm. Indications: Check the instrument to make sure the mirror is stable and the mirror handle is straight before use. Select the right mirror diameter.

## **Nasopharyngeal mirrors different sizes**

### **Specification**

Examination of the post nasal space by a procedure called posterior rhinoscopy, an out-patient procedure. The mirror is warmed and introduced into the oral cavity while the tongue is depressed with a tongue depressor. The mirror is turned upwards in order to examine the post nasal space.

## **Aural speculum different sizes (Set)**

### **Specification**

- **Enhanced Ear Care:** Aural Speculum Set of 3 is designed to aid in the diagnosis and treatment of various ear diseases, ensuring comprehensive ear care.
- **Clear and Direct Vision:** Featuring a straight and long profile, these specula offer direct visual access to the ear canal, improving diagnostic accuracy and treatment precision.
- **Versatile Sizing:** With a range of sizes available, this set of specula can accommodate different patients, ensuring a comfortable and tailored experience for all.
- **Durable Construction:** Crafted from chrome-plated brass, these specula are built for long-term service, guaranteeing durability and reliability in clinical settings.
- **Patient-Focused Design:** The inclusion of three different sizes makes this set suitable for patients of all age groups, further enhancing its versatility and usefulness in medical practice.

*John M. M.*



## Ear Suction different size (Set)

### Specification

- **Medical Grade Stainless Steel:** All cleaner tools are made of medical-grade stainless steel with an anti-slip handle and are easy to clean and sterilize. Ear curette kit uses a unique spring and spiral design that makes the cleaner relieve itching and massage the ear canal to bring you a good cleaning effect.

## Nasal Suction Different Sizes Set

### Specification

- **Stainless Steel Construction:** Crafted from high-quality stainless steel, this instrument is durable, corrosion-resistant, and suitable for repeated sterilization, ensuring longevity and reliability in medical environments.
- **Side-Curved Design:** The side-curved design allows for easy access to the sinus cavities, facilitating smooth and efficient suctioning operations in delicate nasal and sinus regions.
- **Bulbous Tip:** The bulbous tip ensures effective suctioning of fluids and debris, enhancing surgical precision and minimizing the risk of tissue trauma during procedures.

## Suction apparatus

### Specification

- High negative pressure, large flux, low noise.
- Advanced overflow-protection design.
- New design prevents pus and mucus from leaking into the machine.
- Compact, lightweight and easy to carry.
- The phlegm suction machine is suitable for use in a range of medical environments, including home care, clinics, dental offices, and hospitals, catering to different patient needs

*John Vini*



## **Siegel's speculum**

### **Specification**

This speculum is used to perform pneumatic otoscopy where the mobility of the ear drum can be tested. Ear drum mobility can be tested by varying the pressure levels at the external auditory canal and observing the movements of the ear drum in response to these pressure changes.

## **Tuning fork (512 Hz)**

### **Specification**

Produced from Steel Bar for superior performance and consistent frequency accuracy. Each tuning fork is corrosion resistant, lightweight and portable. Perfect to use at home, medical school, or clinics Ideal for hearing, weber and rinne hearing tests, musical instrument tuning, bone conduction tests and more

## **Tuning fork (256 Hz)**


### **Specification**

Produced from Steel Bar for superior performance and consistent frequency accuracy. Each tuning fork is corrosion resistant, lightweight and portable. Perfect to use at home, medical school, or clinics Ideal for hearing, weber and rinne hearing tests, musical instrument tuning, bone conduction tests and more

## **Tuning fork (1024 Hz)**

### **Specification**

Produced from Steel Bar for superior performance and consistent frequency accuracy. Each tuning fork is corrosion resistant, lightweight and portable. Perfect to use at home, medical school, or clinics Ideal for hearing, weber and rinne hearing tests, musical instrument tuning, bone conduction tests and more

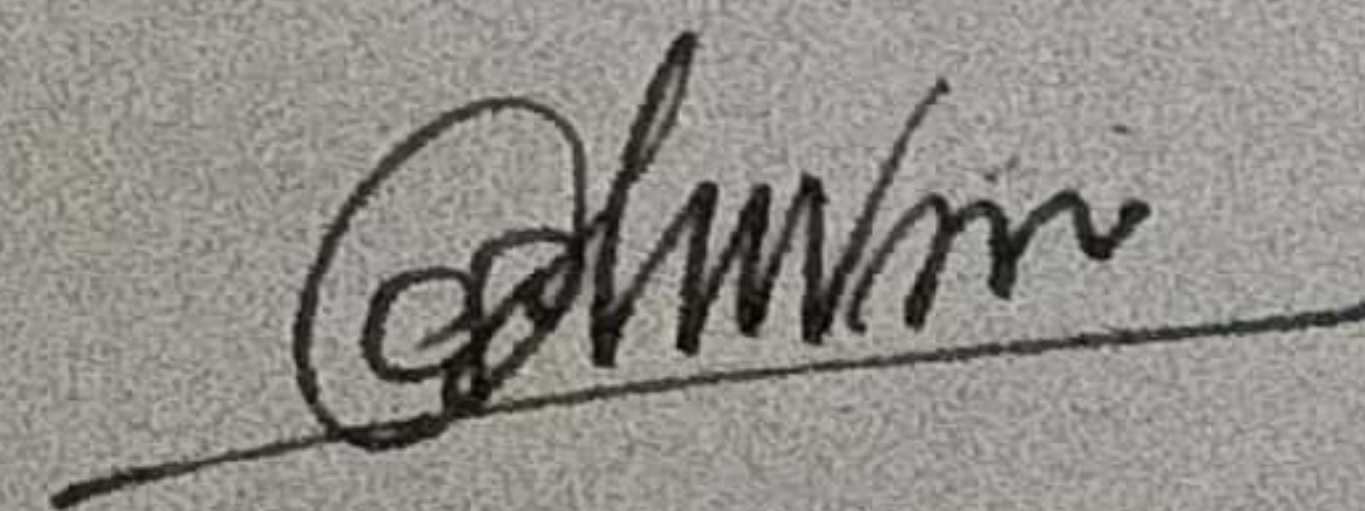



## Otoscope with halogen bulb, rechargeable battery and Siegle attachment

### Specification

Welch allyn 3.5V SureColor LED Otoscope With Rechargeable Handle & Disposable. This is set includes Welch allyn 3.5V SureColor LED Otoscope With Rechargeable Handle, Reusable 4 Specula, 3.5V Rechargeable Battery, Charger, Converter ring in Hard Case. This is Traditional, high-quality otoscopes with a range of illumination options.

### Features

- SureColor LED offers true tissue color and long-lasting performance.
- Wide-angle viewing lens allows for instrumentation under magnification.
- Sealed system for pneumatic otoscopy and accurate diagnosis of otitis media.
- Fiber-optic light has no reflections or obstructions of tympanic membrane views.

### Bayonet forceps

### Specifications

- **Stainless Steel Construction:** Crafted from high-quality stainless steel, ensuring durability, corrosion resistance, and easy sterilization.
- **Bayonet-Shaped Tips:** Designed for improved access and visibility in confined anatomical spaces, facilitating delicate tissue manipulation.
- **Serrated Jaws:** Secure grip on tissues, enhancing precision and reducing the risk of damage during surgery.
- **Ergonomic Handles:** Comfortable and secure grip, minimizing hand fatigue during extended surgical procedures.
- **Versatile Application:** Suitable for a wide range of surgical specialties, contributing to improved surgical outcomes and patient care.

*Edwin*



## Bulls lamp

### Specification

- Metallic Head With Glass
- Adjustable Spring Loaded Arm.
- White Colour Light

Colour	White
Number of Memory Sticks	1
Product Dimensions	30 x 35 x 40 cm
Item Height	40 Centimeters
Item Width	35 Centimeters
Wattage	100 Watts
Lamp wattage	100 Watts

## Head Mirror

### Specification

- A Head Mirror is a simple diagnostic device that is stereotypically worn by physicians or doctors
- These are complete with mirror cover and delivered in packed box.

Devini



## Head Light With LED/Halogen lamp

### Specification

- Easy to use Replaceable battery for prolonged usage
- Rechargeable Battery with cordless design: Extra battery provided
- Long time usage with high power battery : 3 Hours ; USB Charger is provided
- Adjustable Light Intensity ; Lightweight Design for high comfort level

## Jobson Horne probe

### Specification

- Made of high grade stainless steel
- Anti-rust and corrosion resistance. High quality for durable and long-lasting use.
- Most ergonomic designs with impeccable craftsmanship.
- Lightweight with mini size for portable carry.

## Instrument tray


### Specification

- Instruments Tray With Cover (Lid).
- Made From Heavy Gauge Stainless Steel Sheet.
- Size 10" x 8"
- Material: stainless steel tray

## Kidney Tray

### Specification

Made of the highest grade stainless steel (18/8). Crafted without seams allows for easy cleaning. The trays tall lip guards against spills and secures the contents of the tray. The tray can be easily removed for cleaning and sanitizing.

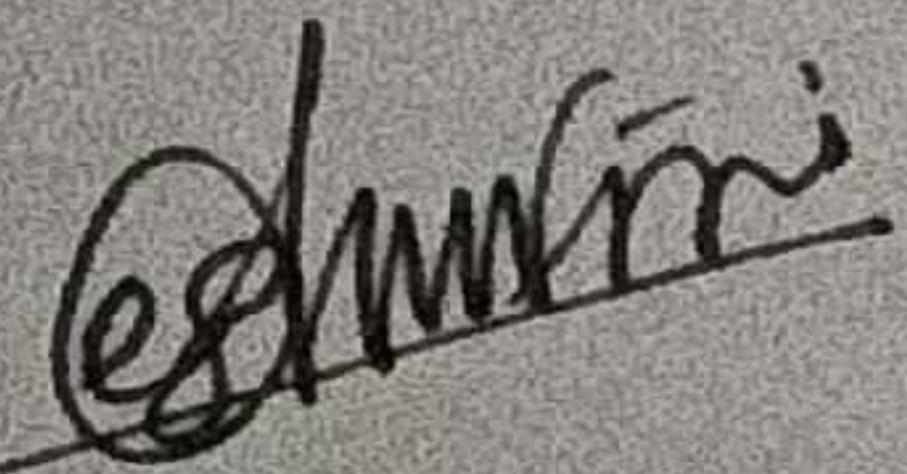

(Dr. Ashvini Somware)  
Assistant Professor  
Department of ENT  
Government Medical College  
Dharashiv